

TEST CERTIFICATE




The following product has been tested by airmid healthgroup ltd as outlined in report(s)
ASCR092207v2

Product Description	DELPHIN DP S8
Manufacturer	PROAIR GmbH
Certificate Number	AHGC: 92207/17/2124/01
Validation Period	13/06/2025
Outline of Test Method	Determination of removal efficiency of Influenza A (H1N1) following aerosolisation of the virus into a 28.5m ³ environmental test chamber. The device operated at the highest speed setting in air cleaner mode during test.
Additional SKUs	DOLPHIN

RESULTS

The DELPHIN DP S8 (in air cleaner mode) was demonstrated to be effective in reducing airborne Influenza A by 99.9% within 20 minutes of operation.

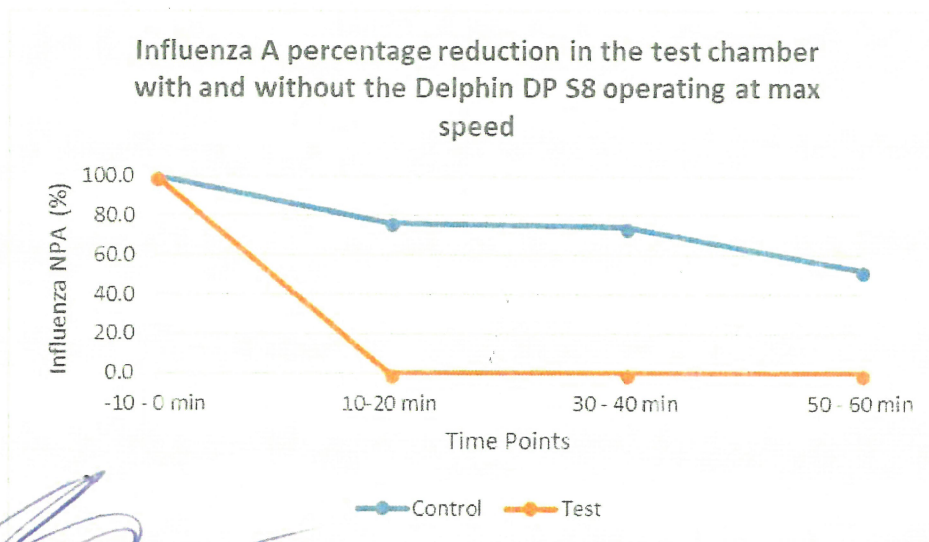

Dr Bruce Mitchell
Chairman/CEO
airmid healthgroup Ltd

24/06/21
Dated

